



## POSTERIOR CROWNS

### PROCERA®, WOL-CERAM®, LAVA®

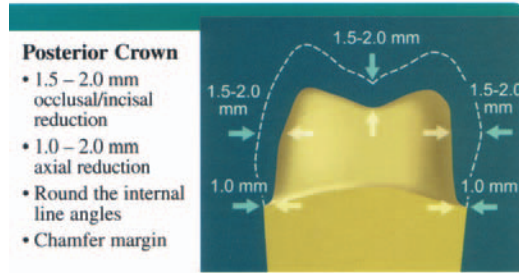


## POSTERIOR BRIDGES

### PROCERA®, WOL-CERAM®, LAVA®

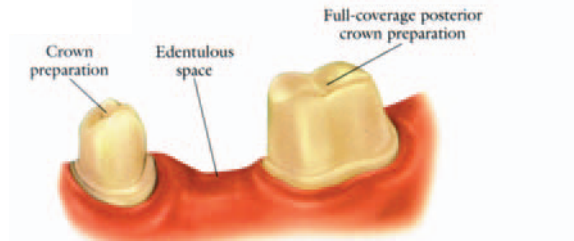


## ANTERIOR CROWNS

### PROCERA®, WOL-CERAM®, LAVA®

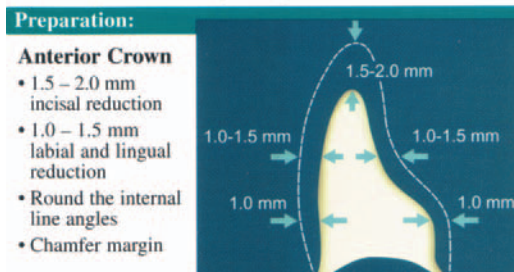

## ANTERIOR BRIDGES

### PROCERA®, WOL-CERAM®, LAVA®

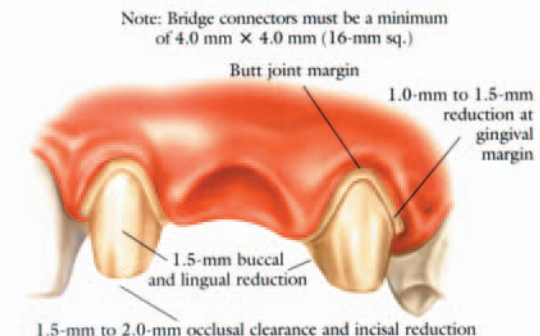

To assure clinical success, the following minimum material thickness is recommended.  
All prepared surfaces must be rounded on all metal-free restorations.